

Optical Analysis

Customer:

Secto Design

Secto Design Oy
Kauppalantie 12
02700 Kauniainen, Finland

Research contract:

ref.no: ta25042013AK.pdf

Target:

Secto Design luminaire, Secto 4231 wall luminaire (shown in Fig. 1).

Handmade design wall light. Crafted in Finland of PEFC-certified formpressed Finnish birch by highly skilled craftsmen.

Finishes of the shade:

Natural birch
White laminated
Black laminated
Walnut veneer

Cable: 240 cm, white, switch on the cable.
Available also with direct wall mounting

Manufacturer: Secto Design
Designer: Seppo Koho



FUNCTIONAL



Fig. 1. Secto 4231. The tested luminaire was with black laminated finish.

Testing time:

The start of the test: 12th June, 2013
The end of the test: 15th August, 2013

Purpose of the test:

The goal of these measurements is to determine the light intensity distribution of the luminaire for lighting design purposes.

Test method:

The light intensity distribution of the luminaire is measured in a goniometer. The goniometer moves a detector of a photometer around the luminaire in one vertical plane and records the

illuminance. The luminaire can be rotated around the vertical axis (horizontal angles).

Vertical angles (around the horizontal axis): $0^{\circ} - 180^{\circ}$, measurement in five-degree increments

Horizontal angles (C-planes): $0^{\circ} - 180^{\circ}$, measurement in 15 degree increments

Validation of the test method:

The light intensity distribution curves provide the designer with important information about the way light is distributed from the luminaire towards e.g. the surrounding walls. This information can be used e.g. with DiaLux modelling software to model how the lighting changes the ambiance in a room.

Performed actions:

Light intensity distribution of Secto 4231 with laminated birch slats was investigated. Sylvania Mini-Lynx Fast-Start, E14 light bulb (600 lm, 840 K) was used during the measurement.

The test arrangement is shown schematically in Fig. 2. The detector of a photometer is mounted in a goniometer. The goniometer can be rotated in a vertical plane. The luminaire is installed in such a way that the centre of the light bulb is placed at the origin of the goniometer.

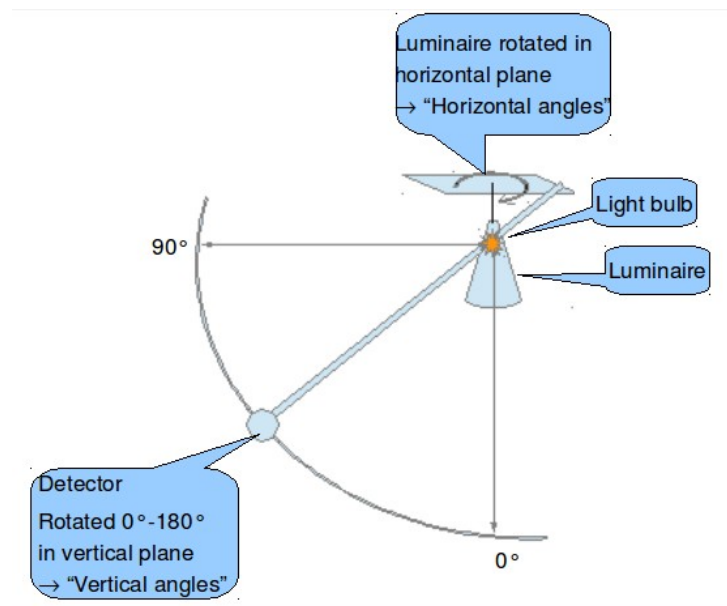


Fig. 2. Scheme of the test arrangement.

Luminaire was rotated in horizontal plane in 15-degree increments in the range of $0^{\circ} - 90^{\circ}$. The measurement in vertical angles was performed in five-degree increments in the range of $0^{\circ} - 180^{\circ}$ in each of these horizontal angles.

Figure 3 shows an example of a light distribution curve. The diagram represents a cut in a plane through a luminaire or lamp and shows the intensity of light emitted in each direction. The centre of the light source is at the origin. The direction 0° is the downward direction and 180° is the upward direction. The straight radial lines in Fig. 3 indicate the angle of the light emitted while the circles are intensity contours. The intensity values of the light distribution curve are scaled to correspond to 1000 lm from the light source (cd/1000 lm). The real cd-value for a specific light bulb can be calculated by multiplying by the 1/1000 of the lumen-value of the bulb. Blue and red curves show light intensity distribution at perpendicular horizontal angles (=C-planes).

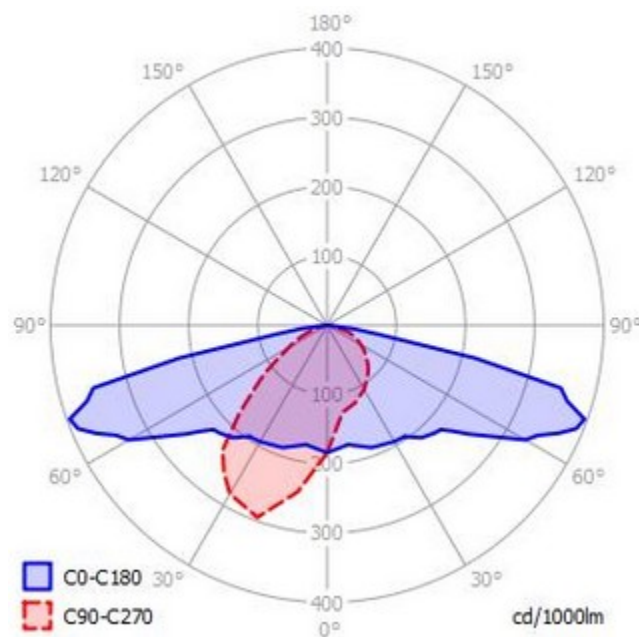


Fig. 3. Light intensity distribution curve. From ref. <http://sourceforge.net/projects/qlumedit/> (14.4.2013)

Light distribution curve of the Secto 4231 luminaire is shown in Fig. 4. The curve was determined using QLumEdit program.

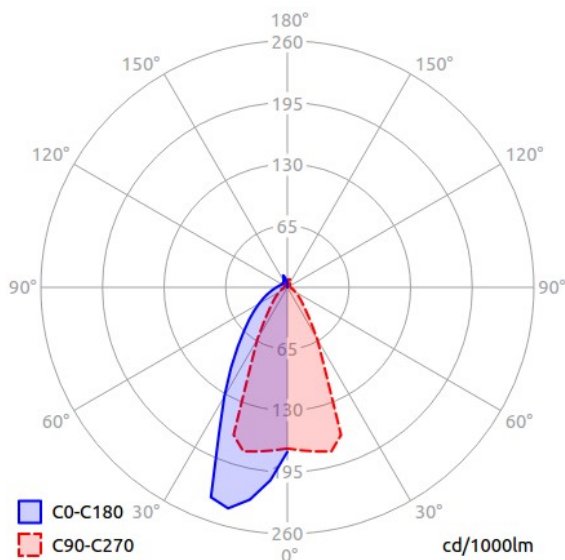


Fig. 4. Light distribution curve of Secto 4231. Light distribution is shown in two perpendicular vertical planes (C-planes).

Used equipment:

Goniometer, No. 59

Photometer, No. 50, calibrated 28th May, 2013, calibration is valid

Analysis/Recommendations:

N/A

Conclusions:

The light intensity curve of the luminaire under test was determined (see **Fig. 4**).

Remarks:

Actions, operations and reporting are in accordance with IEC/ISO 17025 'General requirements for the competence of testing laboratories'.

This review report is based on research report SectoDesignJuselius__tr010513AK.pdf.

Signatures: 

Riitta Perälä

Littoinen 10th June, 2014

